

vacuubrand

Technology for Vacuum Systems

Instructions for use



**VSK 3000
VSP 3000**

Pressure transducer

After sales service: Contact your local dealer or call +49 9342 808-5500

Trademark index:

VACUU•LAN® (US-Reg.No 3,704,401), VACUU•BUS®, VACUU•CONTROL™, chemistry-HYBRID™, Peltronic®, TURBO•MODE™, VARIO® (US-Reg.No 3,833,788), VARIO-SP™, VACUUBRAND® (US-Reg. No 3,733,388) and also the shown company logos are trademarks of VACUUBRAND GMBH + CO KG in Germany and/or other countries.

DE

Achtung: Die vorliegende Betriebsanleitung ist nicht in allen EU-Sprachen verfügbar. Der Anwender darf die beschriebenen Geräte nur dann in Betrieb nehmen, wenn er die vorliegende Anleitung versteht oder eine fachlich korrekte Übersetzung der vollständigen Anleitung vorliegen hat. Die Betriebsanleitung muss vor Inbetriebnahme der Geräte vollständig gelesen und verstanden werden, und alle geforderten Maßnahmen müssen eingehalten werden.  "Sicherheitshinweise für Vakuumgeräte"

EN

Attention: This manual is not available in all languages of the EU. The user must not operate the device if he does not understand this manual. In this case a technically correct translation of the complete manual has to be available. The manual must be completely read and understood before operation of the device and all required measures must be applied.  "Safety instructions for vacuum equipment"

FR

Attention: Le mode d'emploi présent n'est pas disponible dans toutes les langues d'Union Européenne. L'utilisateur ne doit mettre le dispositif en marche que s'il comprend le mode d'emploi présent ou si une traduction complète et correcte du mode d'emploi est sous ses yeux. Le dispositif ne doit pas être mis en marche avant que le mode d'emploi ait été lu et compris complètement et seulement si le mode d'emploi est observé et tous les mesures demandées sont prises.

 «Avis de sécurité pour des dispositifs à vide»

BG

Внимание: Тези инструкции не са преведени на всички езици от ЕО. Потребителят не бива да работи с уреда, ако не разбира инструкциите за ползване. В този случай е необходимо да бъде предоставен пълен технически превод на инструкциите за ползване. Преди работа с уреда е задължително потребителят да прочете изцяло инструкциите за работа.  "Указания за безопасност за вакуумни уреди"

CN

注意：该操作手册不提供所有的语言版本。操作者在没有理解手册之前，不能操作该设备。在这种情况下，需要有一个整个操作手册技术上正确的翻译。在操作该设备前，必须完全阅读并理解该操作手册，必须实施所有需要的测量。

 真空设备的安全信息

CZ

Upozornění :Tento návod k použití není k dispozici ve všech jazycích Evropské unie. Uživatel není oprávněn požít přístroj pokud nerozumí tomuto návodu. V takovém případě je nutno zajistit technicky korektní překlad manuálu do češtiny. Návod musí být uživatelem prostudován a uživatel mu musí plně porozumět před tím než začne přístroj používat. Uživatel musí dodržet všechna příslušná a požadovaná opatření.  "Bezpečnostní upozornění pro vakuové přístroje".

DA

Bemærk: Denne manual foreligger ikke på alle EU sprog. Brugeren må ikke betjene apparatet hvis manualen ikke er forstået. I det tilfælde skal en teknisk korrekt oversættelse af hele manual stilles til rådighed. Manual skal være gennemlæst og forstået før apparatet betjenes og alle nødvendige forholdsregler skal tages.  »Sikkerhedsregler for vakuumudstyr«

EE

Tähelepanu! Käesolev kasutusjuhend ei ole kõigis EL keeltes saadaval. Kasutaja ei tohi seadet käsitseda, kui ta ei saa kasutusjuhendist aru. Sel juhul peab saadaval olema kogu kasutusjuhendi tehniliselt korrektnne tõlge. Enne seadme kasutamist tuleb kuhend läbi lugeda, see peab olema arusaadav ning kõik nõutud meetmed peavad olema rakendatud.  "Ohutusnõuded vaakumseadmetele"

ES

Atención: Este manual no está disponible en todos los idiomas de UE. El usuario no debe manejar el instrumento si no entiende este manual. En este caso se debe disponer de una traducción técnicaicamente correcta del manual completo. El manual debe ser leído y entendido completamente y deben aplicarse todas las medidas de seguridad antes de manejar el instrumento.  "Notas sobre la seguridad para equipos de vacío"

FI

Huomio: Tämä käyttöohje ei ole saatavilla kaikilla EU:n kielillä. Käyttäjä ei saa käyttää laitetta, jos hän ei ymmärrä tätä ohjekirjaa. Tässä tapauksessa on saatavilla oltava teknisesti oikein tehty ja täydellinen ohjekirjan käänös. Ennen laitteen käyttöä on ohjekirja luettava ja ymmärrettävä kokonaan sekä suoritettava kaikki tarvittavat valmistelut ja muut toimenpiteet.  "Vakuumilaitteen turvallisuustiedot"

GR

Προσοχή! : Οι οδηγίες αυτές δεν είναι διαθέσιμες σε όλες τις γλώσσες της Ευρωπαϊκής Ένωσης. Ο χρήστης δεν πρέπει να θέσει σε λειτουργία την συσκευή αν δεν κατανοήσει πλήρως τις οδηγίες αυτές. Σε τέτοια περίπτωση ο χρήστης πρέπει να προμηθευτεί ακριβή μετάφραση του βιβλίου οδηγιών. Ο χρήστης πρέπει να διαβάσει και να κατανοήσει πλήρως τις οδηγίες χρήσης και να λάβει όλα τα απαραίτητα μέτρα πριν θέσει σε λειτουργία την συσκευή.  "Υποδείξεις ασφάλειας για αντλίες κενού"

HR

Pažnja:ove upute ne postoje na svim jezicima Europske Unije. Korisnik nemora raditi sa aparatom ako ne razumije ove upute.U tom slučaju tehnicki ispravni prijevod cijelih uputstava mora biti na raspolaganju. Uputstva moraju biti cijela procitana i razumljiva prije rada sa aparatom i sve zahtijevane mjere moraju biti primjenjene.  "Sigurnosne napomene za vakumske uređaje"

HU

Figyelem! Ez a kezelési utasítás nem áll rendelkezésre az EU összes nyelvén. Ha a felhasználó nem érte jelen használati utasítás szövegét, nem üzemeltetheti a készüléket. Ez esetben a teljes gépkönyv fordításáról gondoskodni kell. Üzembe helyezés előtt a kezelőnek végig kell olvasnia, meg kell értenie azt, továbbá az üzemeltetéshez szükséges összes mérést el kell végeznie.  "A vákuum-készülékekkel kapcsolatos biztonsági tudnivalók"

IT

Attenzione: Questo manuale non è disponibile in tutte le lingue della Comunità Europea (CE). L'utilizzatore non deve operare con lo strumento se non comprende questo manuale. In questo caso deve essere resa disponibile una traduzione tecnicamente corretta del manuale completo. Il manuale deve essere completamente letto e compreso prima di operare con lo strumento e devono essere applicati tutti gli accorgimenti richiesti.  "Istruzioni di sicurezza per apparecchi a vuoto"

JP

注意：この取扱説明書はすべての言語で利用可能ではありません。もしこの取扱説明書を理解できないならば、ユーザーは装置を操作してはなりません。この場合、技術的に正しい翻訳がなされた完全なマニュアルを用意しなければなりません。装置を作動する前にマニュアルを完全に読み、そして理解されなくてはなりません。そして、すべての要求される対策を講じなければなりません。

 真空装置を安全に取り扱うために

KR

주의 : 이 매뉴얼은 모든 언어로 번역되지는 않습니다. 만약 이 매뉴얼의 내용을 충분히 인지하지 못했다면 기기를 작동하지 마십시오. 매뉴얼의 내용을 기술적으로 정확하게 번역한 경우에 이용하십시오. 기기를 사용하기 전에 이 매뉴얼을 충분히 읽고 이해하고 모든 요구되는 사항들을 적용해야 합니다.

 진공 장비에 대한 안전 정보

LT

Dėmesio: šis vadovas nėra pateikiamas visomis ES kalbomis. Naudotojui draudžiama eksplloatuoti įtaisą, jeigu jis nesupranta šio vadovo. Tokiu atveju reikia turėti viso vadovo techniškai taisyklingą vertimą. Vadovą būtina visą perskaityti ir suprasti pateikiamas instrukcijas prieš pradedant eksplloatuoti įtaisą, bei imtis visų reikiamų priemonių.  "Vakuminės įrangos saugos informacija"

LV

Uzmanību: Lietotāja instrukcija nav pieejama visās ES valodās. Lietotājs nedrīkst lietot iekārtu, ja viņš nesaprot lietotāja instrukcijā rakstīto. Šādā gadījumā, ir nepieciešams nodrošināt tehniski pareizu visas lietotāja instrukcijas tulkojumu. Pirms sākt lietot iekārtu, un, lai izpildītu visas nepieciešamās prasības, iekārtas lietotāja instrukcija ir pilnībā jāizlasa un jāsaprot.  "Vakuma iekārtu drošības noteikumi"

NL

Attentie: Deze gebruiksaanwijzing is niet in alle talen van de EU verkrijgbaar. De gebruiker moet niet met dit apparaat gaan werken als voor hem/haar de gebruiksaanwijzing niet voldoende duidelijk is. Bij gebruik van deze apparatuur is het noodzakelijk een technisch correcte vertaling van de complete gebruiksaanwijzing te hebben. Voor het in gebruik nemen van het apparaat moet de gebruiksaanwijzing volledig gelezen en duidelijk zijn en dienen alle benodigde maatregelen te zijn genomen.

 "Veiligheidsvoorschriften voor vacuümapparaten"

PL

Uwaga!! Ta instrukcja nie jest dostępna we wszystkich językach Unii Europejskiej. Użytkownik nie może rozpocząć pracy z urządzeniem dopóki nie przeczytał instrukcji i nie jest pewien wszystkich informacji w niej zawartych. Instrukcja musi być w całości przeczytana i zrozumiana przed podjęciem pracy z urządzeniem oraz należy podjąć wszystkie niezbędne kroki związane z prawidłowym użytkowaniem.

 "Wskazówki bezpieczeństwa do urządzeń próżniowych"

PT

Atenção: Este manual não está disponível em todas as línguas da UE. O usuário não deve utilizar o dispositivo, se não entender este manual. Neste caso, uma tradução tecnicamente correta do manual completo tem de estar disponível. O manual deve ser lido e entendido completamente antes da utilização do equipamento e todas as medidas necessárias devem ser aplicadas.  "Informação de Segurança para Equipamento que funciona a Vácuo"

RO

Atentie: Acest manual nu este disponibil in toate limbile EU. Utilizatorul nu trebuie sa lucreze cu aparatul daca daca nu intlege manualul. Astfel, va fi disponibile o traducere corecta si completa a manualului. Manualul trebuie citit si inteles in intregime inainte de a lucra cu aparatul si a luat toate masurile care se impun.  "Instructiuni de siguranță pentru aparatele de vidare"

RU

Внимание: Эта инструкция по эксплуатации не имеется на всех языках. Потребителю не дозволено эксплуатировать данный прибор, если он не понимает эту инструкцию. В этом случае нужен технически правильный перевод полной инструкции. Прежде чем использовать этот прибор, необходимо полностью прочитать и понять эту инструкцию и принять все необходимые меры.  "Указания по технике безопасности при работе с вакуумными устройствами"

SE

Varning: Denna instruktion är inte tillgänglig på alla språk inom EU. Användaren får inte starta utrustningen om hon/han inte förstår denna instruktion. Om så är fallet måste en tekniskt korrekt instruktion göras tillgänglig. Instruktionen måste läsas och förstås helt före utrustningen tas i drift och nödvändiga åtgärder göras.  "Säkerhetsinformation för vakuumutrustning"

SI

Pozor: Ta navodila niso na voljo v vseh jezikih EU. Uporabnik ne sme upravljati z napravo, če ne razume teh navodil. V primeru nerazumljivosti mora biti na voljo tehnično pravilen prevod. Navodila se morajo prebrati in razumeti pred uporabo naprave, opravljene pa morajo biti tudi vse potrebne meritve.  "Varnostni nasveti za vakumske naprave"

SK

Upozornenie: Tento manuál nie je k dispozícii vo všetkých jazykoch EÚ. Užívateľ nesmie obsluhovať zariadenie, pokiaľ nerozumie tomuto manuálu. V takomto prípade musí byť k dispozícii technicky správny preklad celého manuálu. Pred obsluhou zariadenia je potrebné si prečítať celý manuál a porozumieť mu, a musia byť prijaté všetky opatrenia.  "Bezpečnostné pokyny pre vákuové zariadenia"

TR

Dikkat : Bu kullanım kitabı, tüm dillerde mevcut değildir. Kullanıcı, bu kullanım kitabını anlayamadıysa cihazı çalıştırılmamalıdır. Bu durumda, komple kullanım kitabının, teknik olarak düzgün çevirisinin bulunması gereklidir. Cihazın çalıştırılmasından önce kullanım kitabının komple okunması ve anlaşılması ve tüm gerekli ölçümlerin uygulanması gereklidir.  "Vakumlu cihazlar için güvenlik uyarıları"

Contents

Safety information	7
General information	7
Intended use	7
Connecting the pressure transducer	7
Ambient conditions	8
Operating conditions	8
Safety during operation	8
Maintenance and repair	9
Ex Important information: Equipment marking (ATEX)	10
Technical data	11
Wetted parts	12
Pressure transducer VSK 3000	12
Operation principle of the VSK 3000	12
Changing the vacuum connector	12
Prior to operation	13
VACUU•BUS	13
Pressure transducer VSP 3000	14
Operation principle VSP 3000	14
General information on handling	14
Prior to operation	14
VACUU•BUS	14
During operation	15
Cleaning the pressure transducer	15
Adjustment of the pressure transducer	15
Calibration in the factory	15
Health and safety clearance form	16
EC Declaration of Conformity	17



► DANGER indicates a hazardous situation which, if not avoided, will result in death or serious injury.



► WARNING indicates a hazardous situation which, if not avoided, could result in death or serious injury.



• CAUTION indicates a hazardous situation which, if not avoided, could result in minor or moderate injury.



NOTICE is used to address practices not related to personal injury.



Safety information

General information

WARNING

- ☞ **Read and comply with this manual before installing or operating the equipment.**
- ☞ **Do not use the equipment if it is damaged.**

NOTICE

To operate the pressure transducer VSK 3000 a VACUUBRAND vacuum gauge DCP 3000 or a vacuum controller CVC 3000 or VNC 2 is required. To operate the pressure transducer VSP 3000 a VACUUBRAND vacuum gauge DCP 3000 or a vacuum controller CVC 3000 is required. Remove all packing material, remove the product from its packing-box, remove the protective covers and keep, inspect the equipment.

If the equipment is damaged, notify the supplier and the carrier in writing within three days; state the item number of the product together with the order number and the supplier's invoice number. Retain all packing material for inspection.

Intended use

WARNING

- ☞ Ensure that the individual components are only connected, combined and operated according to their design and as indicated in the instructions for use. Use only **original manufacturer's spare parts and accessories**. Otherwise the safety and performance of the equipment, as well as the electromagnetic compatibility of the equipment might be reduced.
- ☞ The pressure transducers are designed for **ambient and gas temperatures** at the measurement connection of +10°C to +40°C at continuous operation or of up to +80°C for short periods (<5 minutes). Ensure that the maximum permitted gas temperature at the pressure transducer (see "Technical data") is not exceeded.

NOTICE

Use the equipment and all system parts for the intended use only, i.e. for measurement and control of vacuum in vessels designed for that purpose.

Connecting the pressure transducer

WARNING

- ☞ **Avoid uncontrolled overpressure** (e. g. when connecting to a locked or blocked tube system). **Risk of bursting**.

CAUTION

- **Comply with max. permitted pressure** at the pressure transducer, see section "Technical data".
- Connect hoses at the pressure transducer gas tight.
- Ensure stability of the hose connections.
- Check that supply voltage and current conform with the equipment (see rating plate).
- When working with residues, aggressive or condensable media, install a gas washing bottle if necessary.

NOTICE

Avoid high heat supply (e.g., due to hot process gases).

Position device and vacuum connection lines so that no condensate can flow towards the pressure transducer.

Allow the equipment to equilibrate to ambient temperature if you bring it from cold environment into a room prior to operation. Notice if there is water condensation on cold surfaces.

Comply with all applicable and relevant safety requirements (regulations and guidelines). **Implement the required actions and adopt suitable safety measures.**

Ambient conditions**NOTICE**

Ensure that installation is in compliance with the degree of protection, see "Technical data".

Operating conditions**DANGER**

- This device is not approved for operation in potentially explosive atmospheres. **Do not operate the device in potentially explosive atmospheres.**
- Devices without the " Ex " mark on the rating plate are **not approved for operation with dangerous or explosive gases or with potentially explosive or inflammable substances**. Do not operate the device with dangerous or explosive gases or with potentially explosive or inflammable substances.
- Devices bearing the " Ex " mark on their rating plates are **approved for operation with potentially explosive atmospheres** according to their classification II 3G IIC T3 X according to ATEX, but they are **not approved for operation in potentially explosive atmospheres** (see section " Ex Important information: Equipment marking (ATEX)").

CAUTION

- Ensure that the materials of the equipment's wetted parts are compatible with the substances in the vacuum system, see section "Technical data".

Safety during operation**DANGER**

- Adopt suitable measures to prevent the release of dangerous, toxic, explosive, corrosive, noxious or polluting fluids, vapours and gases.
- Prevent any part of the human body from coming in contact with the vacuum.

WARNING**VSK 3000:**

- ☞ **Attention:** At pressures above 1060 mbar the pressure transducer is saturated, the pressure measurement becomes erroneous. **Release pressure immediately. Risk of bursting!**
Maximum permitted pressure: 1.5 bar (absolute).

VSP 3000:

- ☞ **Attention:** Maximum pressure output: $1 \cdot 10^3$ mbar. Pressure values above 1000 mbar can not be read out! **Danger of unnoticed overpressure! Risk of bursting!**
Maximum permitted pressure: 1.5 bar (absolute).

Maintenance and repair**NOTICE**

Return the equipment to the factory for repair. Opening the housing will void any warranty.

In order to comply with law (occupational, health and safety regulations, safety at work law and regulations for environmental protection) products returned to the manufacturer can be **repaired** / DAkkS **calibrated** only when those regulations are complied with.

Returned products will not be repaired or calibrated until the completed health and safety clearance form has been received.

EX Important information: Equipment marking (ATEX)**VACUUBRAND equipment bearing mark (see rating plate)**

 II 3G IIC T3 X
Internal Atm. only
Tech. File Ref.: VAC-EX01

The classification II 3G IIC T3 X according to ATEX is only valid for the inner part (wetted part, pumped gas or vapor) of the equipment. The equipment is not suitable for use in external, potentially explosive atmospheres (environment).

The overall category of the equipment depends on the connected components. If the connected components do not comply with the classification of the VACUUBRAND equipment, the specified category of the VACUUBRAND equipment is no longer valid.

Vacuum pumps and vacuum gauges in category 3 are intended for connection to equipment in which during normal operation explosive atmospheres caused by gases, vapors or mists normally don't occur; or, if they do occur, are likely to do so only infrequently and for a short period only.

Equipment in this category ensures the requisite level of protection during normal operation.

The use of gas ballast or the operation of venting valves is only permitted if thereby explosive atmospheres normally don't occur in the interior of the equipment or, if they do occur, are likely to do so only infrequently and for a short period.

The equipment is marked with "X" (according to EN 13463-1), i.e., restrictions of the operation conditions:

- The equipment is designated for a low degree of mechanical stress and has to be installed in a way so that it cannot be damaged from outside.
Pumping units have to be installed so that they are protected against shocks from the outside and against glass splinters in the event of breakage (implosion).
- The equipment is designated for an ambient and gas inlet temperature during operation of +10 to +40°C. Never exceed these ambient and gas inlet temperatures. If pumping / measuring gases which are not potentially explosive, extended gas inlet temperatures are permissible. See instructions for use, section "Gas inlet temperatures" or "Technical data"

After any intervention at the equipment (e.g., repair / maintenance) the ultimate vacuum of the pump has to be checked. Only if the pump achieves its specified ultimate vacuum is the pump's leak rate low enough to ensure that no explosive atmospheres will occur in the interior of the equipment.

After any intervention at the vacuum sensor, the leak rate of the equipment has to be checked.



Attention: This manual is not available in all languages of the EU. The user must not operate the device if he does not understand this manual. In this case a technically correct translation of the complete manual has to be available. The manual must be completely read and understood before operation of the device. All specified measures must be applied, or else must be replaced by equivalent measures at the user's own risk.

Technical data

Type	VSK 3000	VSP 3000
Measuring principle	ceramic diaphragm (alumina), capacitive, absolute pressure, gas type independent	thermal conductivity according to Pirani, dependent on gas type
Measuring range (absolute)	1060 mbar - 0.1 mbar (795 Torr - 0.1 Torr)	$1 \cdot 10^3$ mbar - $1 \cdot 10^{-3}$ mbar ($7.5 \cdot 10^2$ Torr - $1 \cdot 10^{-3}$ Torr)
Resolution	0.1 mbar	10% of displayed decade
Measurement uncertainty (absolute) after careful adjustment and at constant temperature	<±1 mbar (0.75 Torr) / ±1 digit	$1 \cdot 10^1$ mbar - $1 \cdot 10^{-2}$ mbar ($1 \cdot 10^1$ Torr - $1 \cdot 10^{-2}$ Torr): ±15% of displayed value
Maximum permissible pressure at pressure transducer	1.5 bar (1125 Torr) absolute	
Maximum permissible temperature of gaseous media at measurement connection*	continuous operation: 40°C, for short periods (< 5 minutes): up to 80°C	
Temperature coefficient	<±0.07 mbar/K (0.05 Torr/K)	-
Ambient temperature range (operation)	10°C to +40°C	
Ambient temperature range (storage)	-10°C to +60°C	
Permitted relative atmospheric moisture during operation (no condensation)	30% to 85%	
Range of supply voltage (via VACUU•BUS)	6-30 VDC / 5 mA	18-30 VDC / 65mA
Degree of protection IEC 529	IP 54	
Communication	VACUU•BUS	
Weight	185 g 180 g 178 g	180 g 185 g -
with small flange		
with hose nozzle		
with tubing connection		
Housing dimensions	diameter length with vacuum connection	60 mm 58 mm 97 mm -
diameter		
length with vacuum connection		
Vacuum connection	small flange DN 16 or hose nozzle 6/10 mm or connection for PTFE tubing DN 8/10 mm	small flange DN 16 and screw-in hose nozzle 6/10 mm
Internal volume of measurement chamber	with small flange: 4.1 cm ³ with hose nozzle: 4.4 cm ³ with tubing connection: 3.5 cm ³	2.9 cm ³ with hose nozzle: 2.5 cm ³
Cable length	approximately 2.0 m	

* if using potentially explosive atmospheres (only VSK 3000): 50 °F to 104 °F (+10°C to +40°C)

We reserve the right for technical modification without prior notice!

Wetted parts

Components	Wetted materials
VSK 3000	
Sensor	aluminium oxide ceramics
Sensor housing, measurement chamber	PPS, glass fibre
Seal at sensor	chemically resistant fluoroelastomer
Hose nozzle	PP
Clamping ring	PA
Small flange	stainless steel or PP
VSP 3000	
Sensor	aluminium oxide ceramics
Sensor housing, measurement chamber, small flange	PBT, glass fibre / PUR
Hose nozzle / O-ring	PPS, glass fibre / FPM

We reserve the right for technical modification without prior notice!

Pressure transducer VSK 3000


Operation principle of the VSK 3000

The VSK 3000 is equipped with a capacitive pressure transducer with ceramic diaphragm to measure the actual pressure **independent of the gas type** and depending on the vacuum, i. e. **absolute**.

Changing the vacuum connector


Installing the hose nozzle:

Unscrew the flange (using a 17 mm open-end wrench, if necessary) to expose the compression fitting (1). Slip the compression nut, and then the ferrule, onto the smooth end of the supplied hose nozzle (2). Slide the smooth end of the hose nozzle onto the compression fitting on the VSK 3000 gauge head, and tighten the compression nut firmly finger-tight (3).

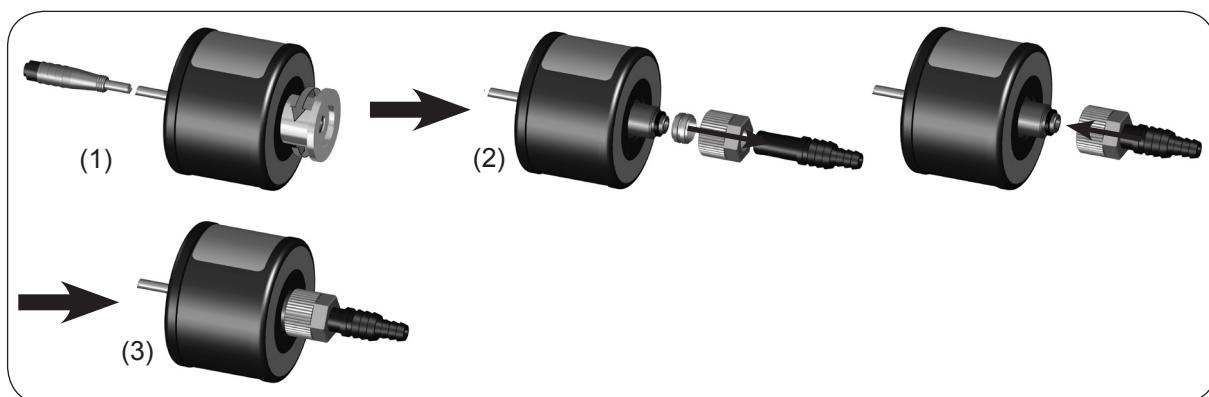

Installing the PTFE-tubing connection (PTFE-tubing ID: 8mm, OD: 19mm):

Unscrew the flange (using a 17 mm open-end wrench, if necessary) to expose the compression fitting (1). Slip the compression nut, and then the ferrule, onto the PTFE-tubing (2). Slide the PTFE-tubing onto the compression fitting on the VSK 3000 gauge head, and tighten the compression nut firmly finger-tight (3).

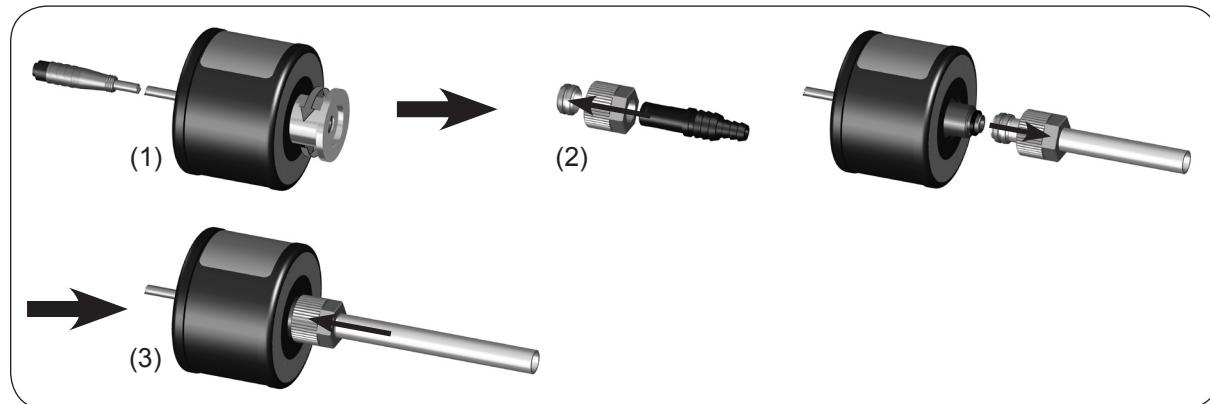**Prior to operation**

- Connect gauge head by means of the VACUU•BUS line to a controller CVC 3000 or VNC 2 or to a vacuum gauge DCP 3000.
- Connect the gauge head to the vacuum chamber by means of the small flange connection or a hose connection. Avoid contamination (oil/oil mist) of the gauge head when generating the vacuum with an oil-sealed vacuum pump.
- ☞ Do not mount the gauge head directly at the oil-sealed pump but close to the vacuum process. The diameter of the vacuum lines should be as large as possible.
- ☞ Inside a vacuum system where evaporation occurs (e.g., rotary evaporator) the vacuum is not uniform (e.g., a condenser acts as pump or the vacuum in the pipeline is lower than in the system). Therefore choose carefully the position where to connect the gauge head.
- ☞ Condensate and deposits at the gauge head falsify the measurement result.
- ☞ If residues occur or when working with aggressive or condensable substances, install a gas washing bottle in front of the pressure gauge head.
- Mount the gauge head in such a position that condensate can not flow into it.**
- ☞ If necessary, clean the gauge head.

VACUU•BUS

Readout of the pressure transducer via VACUU•BUS line by the controller CVC 3000 or VNC 2 or by the vacuum gauge DCP 3000 using VACUU•BUS protocol (see instructions for use of vacuum controllers CVC 3000 or VNC 2 or of vacuum gauge DCP 3000). Maximum cable length inside buildings: 30m. Extension cable VACUU•BUS 2m: order-no. 612552.

With the devices CVC 3000 and DCP 3000 it is possible to adjust and to configure the pressure transducer VSK 3000. (A configuration of the VSK 3000 e.g., to a different VACUU•BUS address, is required if more than one pressure transducer are connected to a CVC 3000 or DCP 3000.)

Additional instructions for use regarding the configuration of pressure transducers or other VACUU•BUS components are available upon request.

Pressure transducer VSP 3000

Operation principle VSP 3000

The pressure transducer VSP 3000 relies on the fact that the thermal conductivity of the residual gas in the vacuum chamber is a measure for the gas pressure. The thermal conductivity of gases is proportional to the pressure within a certain range and is related to the molecular mass.

The thermal conductivity of gases and vapours varies with their molecular mass. Therefore the pressure measurement is dependent on the gas type. The pressure transducer has been adjusted for air at the factory.

- ☞ Pressure of gases with similar mass, such as O₂ or CO, can be read off directly within the uncertainty of the measurement.
- ☞ With gases of lower or higher mass (H₂, He, Ar, CO₂) it is recommended to readjust the VSP 3000 using the gas to be measured.

General information on handling

The pressure transducer VSP 3000 which has been developed particularly for use in chemical laboratories is a pressure sensor working in the fine vacuum range.

Allow the VSP 3000 a period of approx. 20 minutes to warm up and to meet its specifications. Even in case of the controller or vacuum gauge being switched off, the VSP 3000 stays ready for operation. To de-energize the pressure transducer, unplug either its VACUU•BUS line or the power supply of the controller or vacuum gauge.

NOTICE

The interior of the pressure transducer is highly sensitive! Do not insert fingers or tools into the measuring chamber.

Prior to operation

- Connect gauge head by means of the VACUU•BUS line to a controller CVC 3000 or to a vacuum gauge DCP 3000.
- Connect the gauge head to the vacuum chamber by means of the small flange connection or a hose connection. Avoid contamination (oil/oil mist) of the gauge head when generating the vacuum with an oil-sealed vacuum pump.
- ☞ Do not mount the gauge head directly at the oil-sealed pump but close to the vacuum process. The diameter of the vacuum lines should be as large as possible.
- ☞ Inside a vacuum system where evaporation occurs (e.g., rotary evaporator) the vacuum is not uniform (e.g., a condenser acts as pump or the vacuum in the pipeline is lower than in the system). Therefore choose carefully the position where to connect the gauge head.
- ☞ Condensate and deposits at the gauge head falsify the measurement result.
- ☞ If residues occur or when working with aggressive or condensable substances, install a gas washing bottle in front of the pressure gauge head.
- ☞ **Mount the gauge head in such a position that condensate can not flow into it.**
- ☞ If necessary, clean the pressure transducer.

Recommended orientation: Vertically with vacuum connection pointing downwards. If mounting the VSP 3000 in any other orientation, a readjustment is recommended.

VACUU•BUS

Readout of the pressure transducer via VACUU•BUS line by the controller CVC 3000 or by the vacuum gauge DCP 3000 using VACUU•BUS protocol (see instructions for use of vacuum controllers CVC 3000 or vacuum gauge DCP 3000). Maximum cable length inside buildings: 30m. Extension cable VACUU•BUS 2m: order-no. 612552.

With the devices CVC 3000 and DCP 3000 it is possible to adjust and to configure the pressure transducer VSP 3000. (A configuration of the VSP 3000 e.g., to a different VACUU•BUS address, is required if more than one pressure transducer are connected to a CVC 3000 or DCP 3000.)

Additional instructions for use regarding the configuration of pressure transducers or other VACUU•BUS components are available upon request.

During operation

Over the whole measuring range the pressure reading is indicated in exponential notation.

Cleaning the pressure transducer

NOTICE

Attention: Never use a spiky or sharp-edged tool to clean the pressure transducer.

VSK 3000: Never touch the ceramic diaphragm at the back of the measuring chamber with hard objects!

VSP 3000: The interior of the pressure transducer is highly sensitive! Do not insert fingers or tools into the measuring chamber.

Clean a contaminated pressure transducer as follows:

- Fill the measuring chamber with a solvent (e.g., benzene) and allow sufficient cleaning time. Observe all regulations concerning usage and disposal of solvents!
- Drain the solvent and dispose of in accordance with regulations, repeat cleaning if necessary.
- Rinse the measuring chamber several times with alcohol in order to remove all solvent residues.
- Allow the pressure transducer to dry.
- Readjust the pressure transducer if necessary.

Adjustment of the pressure transducer

For adjusting the pressure transducer, either a vacuum controller CVC 3000 or a vacuum gauge DCP 3000 is required,

Depending on operation conditions, accuracy requirements and the type of application, an inspection and a readjustment may be necessary. It may also be required to readjust the pressure transducer after it has been cleaned. (See the manual of the vacuum controller CVC 3000 or of the vacuum gauge DCP 3000 for instructions on adjustment. Download the latest version at www.vacuubrand.com)

Calibration in the factory

Control of measuring equipment

The **VACUUBRAND DAkkS calibration laboratory** is accredited by the Deutsche Akkreditierungsstelle GmbH (national accreditation body of the Federal Republic of Germany) for the measurable variable **pressure in the pressure range from $7.5 \cdot 10^{-4}$ Torr to 975 Torr (10^{-3} mbar to 1300 mbar)** in accordance with the general criteria for the operation of testing laboratories defined in the DIN EN ISO/IEC 17025:2000 series of standards (accreditation number D-K-15154-01). The DAkkS is signatory to the multilateral agreements of the European cooperation for Accreditation (EA) and of the International Laboratory Accreditation Cooperation (ILAC) for the mutual recognition of calibration certificates.

Rely on calibration in the VACUUBRAND calibration laboratory:

- To meet the requirements of the DIN ISO 9000ff and 10012 series of standards regarding the calibration of inspection, measuring and test equipment at specified intervals.
- To document that the vacuum gauges calibrated are traceable to national standards of the PTB (Physikalisch-Technische Bundesanstalt; German national institute for science and technology and the highest technical authority of the Federal Republic of Germany for the field of metrology and certain sectors of safety engineering).

Health and safety clearance form



Devices will not be accepted for any handling before we have received this declaration.

Please read and comply with "Notes on return to the factory".

Oil filled pumps: Drain oil prior to shipping absolutely!

1. Device (Model): 2. Serial no.:

3. Reason for return / malfunction:

.....
4. Has the device been used in a copper process step (e.g., semiconductor production).

yes no

5. Substances (gases, liquids, solids) in contact with the device / which have been pumped:

.....
.....
.....

6. Prior to return to the factory the device has been decontaminated.

yes no

Description of the decontamination method and the test / verification procedure:

.....
.....

7. The device is free of hazardous, harmful substances.

yes no

8. Protective measures required for VACUUBRAND employees:

.....
9. If the paint is damaged, we wish a repaint or a replacement of parts for reason of appearance (repaint and replacement at customer's expense).

yes no

10. Legally binding declaration

We assure for the returned device that all substances, which have been in contact with the device are listed in section 5 and that the information is complete and that we have not withheld any information. We declare that all measures - where applicable - have been taken listed in section "Return to the factory".

By our signature below, we acknowledge that we accept liability for any damage caused by providing incomplete or incorrect information and that we shall indemnify VACUUBRAND from any claims as regards damages from third parties. We are aware that as expressed in § 823 BGB (Public Law Code of Germany) we are directly liable for injuries or damages suffered by third parties, particularly VACUUBRAND employees occupied with handling/repairing the product.

Shipping of the device must take place according to regulations.

Name: Signature:

Job title: Company's seal:

Date:

Release for repair grant by VACUUBRAND (date / signature):



**EG-Konformitätserklärung
EC Declaration of Conformity
Déclaration CE de conformité**

Hersteller / Manufacturer / Fabricant:

VACUUBRAND GMBH + CO KG · Alfred-Zippe-Str. 4 · 97877 Wertheim · Germany

Hiermit erklärt der Hersteller, dass das Gerät konform ist mit den Bestimmungen der Richtlinie 2004/108/EG.

Hereby the manufacturer declares that the device is in conformity with the directive 2004/108/EC.
Par la présente, le fabricant déclare, que le dispositif est conforme à la directive 2004/108/CE.

Druckaufnehmer / Pressure transducer / Capteur de pression

Typ / Type / Type: VSK 3000 / VSP 3000

Artikelnummer / Order number / Numéro d'article: 636657 / 636163, 2614277, 2614436, 2614681

Seriennummer / Serial number / Numéro de série: Siehe Typenschild / See rating plate / Voir plaque signalétique

Die Maschine ist konform mit weiteren Richtlinien / The machinery is in conformity with other directives / La machine est conforme à d'autres directives:

94/9/EG (nur / only / seulement: VSK 3000)

Angewandte harmonisierte Normen / Harmonized standards applied / Normes harmonisées utilisées:

DIN EN 12100:2004

nur / only / seulement VSK 3000: DIN EN 1127-1:2011, DIN EN 13463-1:2009

Bevollmächtigter für die Zusammenstellung der technischen Unterlagen / Person authorised to compile the technical file / Personne autorisée à constituer le dossier technique:

Dr. J. Dirscherl · VACUUBRAND GMBH + CO KG · Alfred-Zippe-Str. 4 · 97877 Wertheim · Germany

Wertheim, 22.07.2014

Ort, Datum / place, date / lieu, date

(Dr. F. Gitmans)

Geschäftsführer / Managing director / Gérant

ppa.

(Dr. J. Dirscherl)

Technischer Leiter / Technical Director / Directeur technique

VACUUBRAND GMBH + CO KG
Alfred-Zippe-Str. 4 · 97877 Wertheim
T +49 9342 808-0 · F +49 9342 808-5555
E-Mail: info@vacuubrand.com
Web: www.vacuubrand.com

Disclaimer: Our technical literature is only intended to inform our customer. The validity of general empirical values and results obtained under test conditions for specific applications depend on a number of factors beyond our control. It is therefore strictly the users' responsibility to very carefully check the validity of application to their specific requirements. No claims arising from the information provided in this literature will, consequently, be entertained.

